# Vibro-Meter

CA 306

# Piezoelectric Accelerometer

#### **FEATURES**

- Designed for high temperature gas turbine applications
- Continuous operation up to 500°C
- High output of 50 pC/g
- Improved transverse frequency resonance
- 4-hole mounting according to ARINC Characteristic 554
- Certified for use in potentially explosive atmospheres
- Construction: Hermetically welded Inconel 600 superalloy
- Frequency response: 5 Hz to 3 000 Hz









# **DESCRIPTION**

The CA 306 series of high temperature accelerometers has been designed specifically for gas turbine applications.

The accelerometers feature a rugged design with hermetically sealed connectors.

An integral mineral insulated (MI) cable with stainless

steel overbraid ensures signal integrity even in the most hostile environments.

The differential output signal minimizes noise pick-up due to electrical ground potentials.

A version with side connector is available when an integral cable is not required.



The information contained in this document may be subject to export control regulations of the European Community, USA or other countries. each recipient of this document is responsible for ensuring that the transfer or use of any information contained in this document complies with all relevant export control regulations. ECN N/A.



#### **SPECIFICATIONS**

**GENERAL** 

Input power requirements : None

Signal transmission : 2 pole system insulated from casing, charge output

: Charge amplifier Signal processing

**OPERATING** 

(at 23°C ± 5°C)

: 50 pC/g ± 5% Sensitivity (at 120 Hz) Dynamic measuring range (random) : 0.01 g to 100 g peak Overload capacity (spikes) : Up to 200 g peak

: ±1% over dynamic measuring range Linearity

Transverse sensitivity : <5% Resonant frequency : >15 kHz

Frequency response (typical) : ± 5% between 5 and 3 000 Hz (lower cut-off frequency is determined by

electronics used)

: Min.  $10^9~\Omega$  pole-ground Min.  $10^9~\Omega$  pole-pole Internal insulation resistance

#### **ENVIRONMENTAL**

Temperature range

• Transducer and cable : -55°C to 500°C (VM-Lemo connector) (-65°C to 125°C)

: ± 10% between -55°C and 500°C Temperature response

Shock acceleration : <1000 g peak (1 ms half sine wave) along sensitive axis

Base strain sensitivity : ≤10<sup>-4</sup> g/με

Corrosion, humidity : Inconel 600, hermetically welded

Use in explosive atmospheres:

KEMA 04 ATEX 1294 II 1 G (Zones 0, 1, 2) Ex ia IIC T6 to T510 • EC type examination certificate

For specific parameters of the mode of protection concerned and special conditions for safe use, please refer tothe "EC type examination certificate" that is available from Vibro-Meter SA on demand.

· cCSAus standard : Certificate 1550831,

Class I, Division 1, Groups A, B, C and D

Ex ia T6 to T1

**MECHANICAL** 


: Four 6-32 NC bolts (according to ARINC 554) or M3.5 bolts, screw torque Mounting

5 Nm. No need for electrical insulation of mounting surface.

#### **CALIBRATION**


Dynamic calibration at factory at 5 g peak and 120 Hz (23°C). No subsequent calibration necessary.

#### **TYPICAL RESPONSE CURVES**

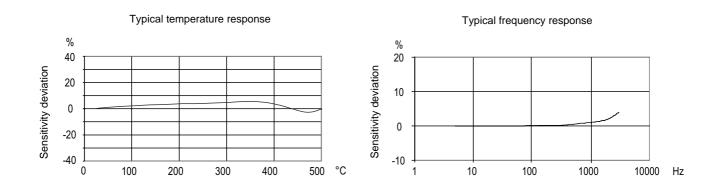

#### **DIMENSIONS AND ORDERING INFORMATION**


#### **CA 306 Version 011**

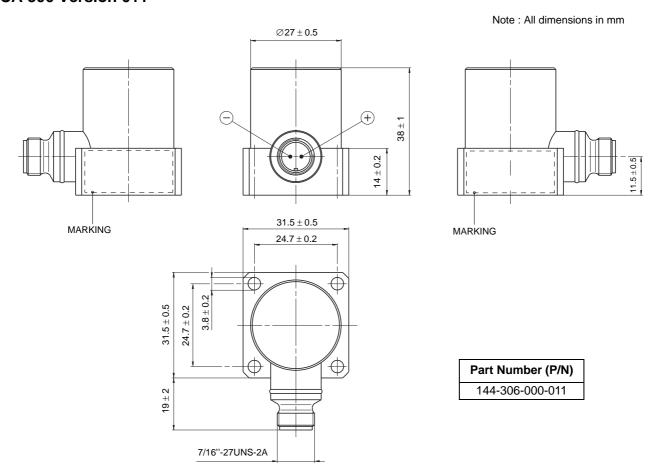


# **DIMENSIONS AND ORDERING INFORMATION (Continued)**

# CA 306 Version 1XX

Note: All dimensions in mm

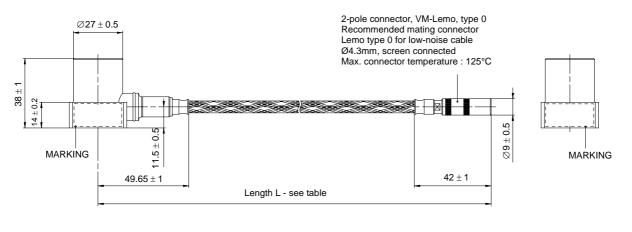

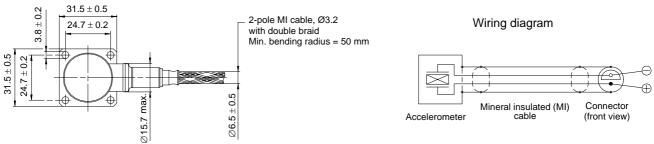



Part Number (P/N)	Length L in mm
144-306-000-111	3000 ± 100
144-306-000-121	6000 ± 150
144-306-000-131	9000 ± 200
144-306-000-141	12000 ± 200

# **DIMENSIONS AND ORDERING INFORMATION** (Continued)

#### CA 306 Version 3XX

Note: All dimensions in mm

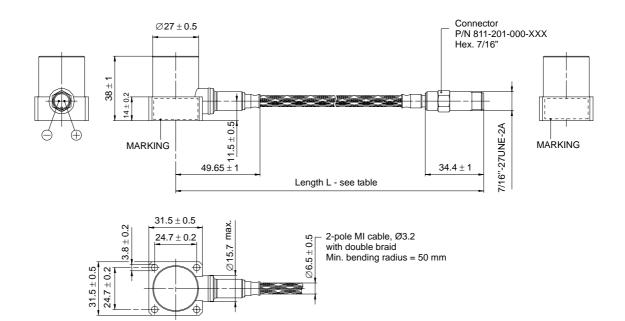



Part Number (P/N)	Length L in mm
144-306-000-311	3000 ± 100
144-306-000-321	6000 ± 150
144-306-000-331	9000 ± 200
144-306-000-341	12000 ± 200

Vibro-Meter



All statements, technical information, drawings, performance rates and descriptions in this document, whilst stated in good faith, are issued for the sole purpose of giving an approximate indication of the products described in them, and are not binding on Vibro-Meter SA unless expressly agreed in writing. Before acquiring this product, you must evaluate it and determine if it is suitable for your intended application. Unless otherwise expressly agreed in writing with Vibro-Meter, you assume all risks and liability associated with its use. Any recommendations and advice given without charge, whilst given in good faith, are not binding on Vibro-Meter.

Vibro-Meter takes no responsibility for any statements related to the product which are not contained in a current Vibro-Meter publication, nor for any statements contained in extracts, summaries, translations or any other documents not authored by Vibro-Meter. We reserve the right to alter any part of this publication without prior notice.

In this publication, a dot (.) is used as the decimal separator and thousands are separated by spaces. Example: 12 345.678 90.

Sales offices Your local agent Head office

Vibro-Meter has offices in more than 30 countries. For a complete list, please visit our website.

Vibro-Meter SA Rte de Moncor 4 P.O. Box CH-1701 Fribourg Switzerland

Tel: +41 26 407 11 11 Fax: +41 26 407 13 01

www.vibro-meter.com



